CoreMass Laboratories

Certificate of Analysis

Independent analytical testing · Alberta, Canada · info@coremasslaboratories.com

REPORT NO.
VOLT3211801

ISSUED
Nov 13, 2026

SAMPLE
BPC-157 / TB-500
5 mg + 5 mg vial · Wolverine blend

HPLC PURITY
99.70%

IDENTITY
Confirmed

NET CONTENT
5.71 + 5.82 mg



Vial as received

CLIENT	Volta Peptides
ORDER ID	321026
LOT / BATCH	VPWV10100
LABEL CLAIM	5 mg + 5 mg
APPEARANCE	White lyophilized powder
VIALS RECEIVED	2
RECEIVED	Nov 11, 2026
ANALYSIS COMPLETED	Nov 13, 2026


TEST PANELS

✓ All 7 requested panels meet specification or are reported


	PANEL AND METHOD	SPECIFICATION	RESULT	STATUS
01	**Purity** Reversed-phase HPLC with UV detection, area percent	≥ 98.0%	**99.70%**	✓ Conforms
02	**Identity** HPLC coupled with electrospray mass spectrometry	Matches both peptides	**Confirmed** BPC-157 and Thymosin β4	✓ Conforms
03	**Net Peptide Content** Quantified against calibrated reference-standard curves	Report only	**5.71 + 5.82 mg** BPC-157 + Thymosin β4	Reported
04	**Bacterial Endotoxin** Limulus Amebocyte Lysate (LAL) assay per USP <85>	Pass	**Pass**	✓ Conforms
05	**Microbial Screen** Polymerase chain reaction, microbial DNA	Not detected	**Not detected**	✓ Conforms
06	**Elemental Impurities** ICP-MS · As, Cd, Pb, Hg	Below limits	**Pass**	✓ Conforms
07	**Fentanyl Screen** Targeted fentanyl screen	Not detected	**Not detected**	✓ Conforms

CHROMATOGRAM AND MASS CONFIRMATION

HPLC-UV · PDA BPC-157 5.38 min · Thymosin β4 6.35 min · purity 99.70%

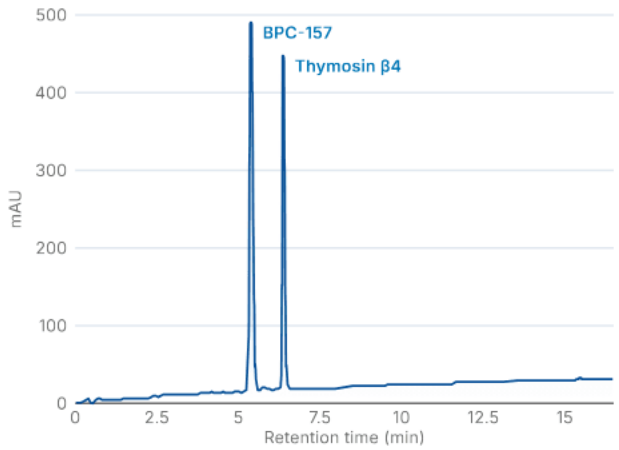

LC-MS · ESI positive Charge states for each peptide

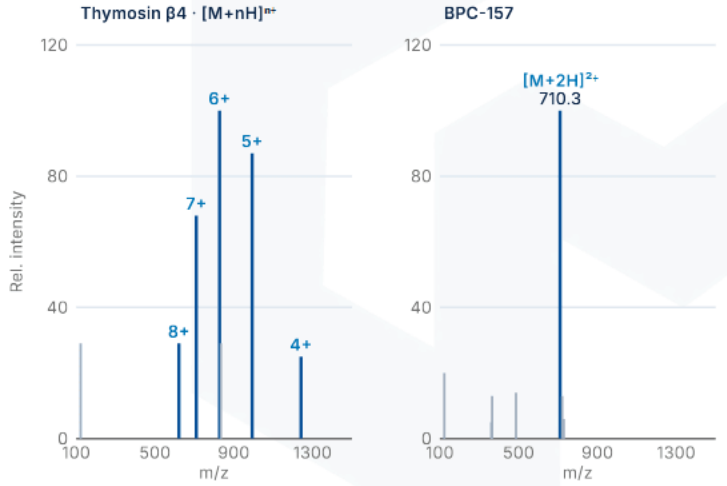

Verify this report

Scan the QR code or enter the report number at coremasslaboratories.com. Full panel data is on page 2.

Results relate only to the sample as received. Sample names, lot numbers and label claims are supplied by the client and are not independently verified. Research-use laboratory testing, not a clinical or diagnostic service. CoreMass Laboratories does not manufacture, sell or endorse any tested material. Reproduce only in full.

CoreMass Laboratories

Analytical Detail

REPORT NO.
VOLT3211801
BPC-157 / TB-500 · Nov 13, 2026

01 Purity

✓ Conforms

Reversed-phase HPLC with UV detection, area percent

Sample 1 **99.70%** Sample 2 **99.72%**

Sample	Purity (area %)	Status
Sample 1	99.70	Pass
Sample 2	99.72	Pass

Combined BPC-157 and Thymosin β4 peak area as a share of total integrated peak area.

02 Identity

✓ Conforms

HPLC coupled with electrospray mass spectrometry

Target	Result	Status
BPC-157	Confirmed	Pass
Thymosin β4	Confirmed	Pass

Identity confirmed as BPC-157 and Thymosin β4 by LC-MS.

03 Net Peptide Content

Reported

Quantified against calibrated reference-standard curves

Label claim **5 mg + 5 mg**

Vial	BPC-157	Thymosin β4
Vial 1	5.71 mg (114.2%)	5.82 mg (116.4%)
Vial 2	5.59 mg (111.8%)	5.62 mg (112.4%)

Measured content of each peptide per vial, with percent of its 5 mg label claim.

04 Bacterial Endotoxin

✓ Conforms

Limulus Amebocyte Lysate (LAL) assay per USP <85>

Assay sensitivity **≤ 0.05 EU/mL** Replicates **2**

Measure	Assay sensitivity	Status
Replicate 1	≤ 0.05 EU/mL	Pass
Replicate 2	≤ 0.05 EU/mL	Pass

Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85> under validated laboratory conditions.

05 Microbial Screen

✓ Conforms

Polymerase chain reaction, microbial DNA

Assay **PCR, common microbial contaminants**

Target	Result	Status
Microbial DNA	No detectable microbial DNA	Pass

Detects microbial DNA. Does not distinguish live from dead organisms and is not a USP <71> culture sterility test.

06 Elemental Impurities

✓ Conforms

ICP-MS · As, Cd, Pb, Hg

Elements **As, Cd, Pb, Hg**

Element	Result	Status
Arsenic (As)	Below reporting/specification limit	Pass
Cadmium (Cd)	Below reporting/specification limit	Pass
Lead (Pb)	Below reporting/specification limit	Pass
Mercury (Hg)	Below reporting/specification limit	Pass

Arsenic, cadmium, lead and mercury were below reporting/specification limits.

07 Fentanyl Screen

✓ Conforms

Targeted fentanyl screen

Analyte	Result	Status
Fentanyl	No fentanyl detected	Pass

No fentanyl detected.

Reading this report

- **Conforms** means the result met the listed specification. **Reported** means a measured value with no pass or fail limit.
- Purity is the share of detected material that is the target compound. Net content is the measured amount in the vial. A sample can be highly pure and still hold less than its label states.
- ND means not detected, below the limit of detection (LOD). LOQ is the limit of quantification.
- Endotoxin and PCR testing use their own sealed vials, listed on each panel.

SHA-256 REPORT HASH

1f1b9c8edde9ea8c5a25559c2f797011bdab3699d117a71c1813659d7a24c983

Original issue. Results relate only to the sample as received. Sample names, lot numbers and label claims are supplied by the client and are not independently verified. Research-use laboratory testing, not a clinical or diagnostic service. CoreMass Laboratories does not manufacture, sell or endorse any tested material. Reproduce only in full.